


NON-STANDARD AVSU MODULE SURFACE SPECIFICATION SHEET FOR 5 OR MORE GASES.

Sales Contract No		Customer Order No.	
Project Ref.		Delivery Date Requested	
Qty		Batch No.	
Customer			

Alarm centre height must not exceed 1800mm from the finished floor height (HTM 02-01)

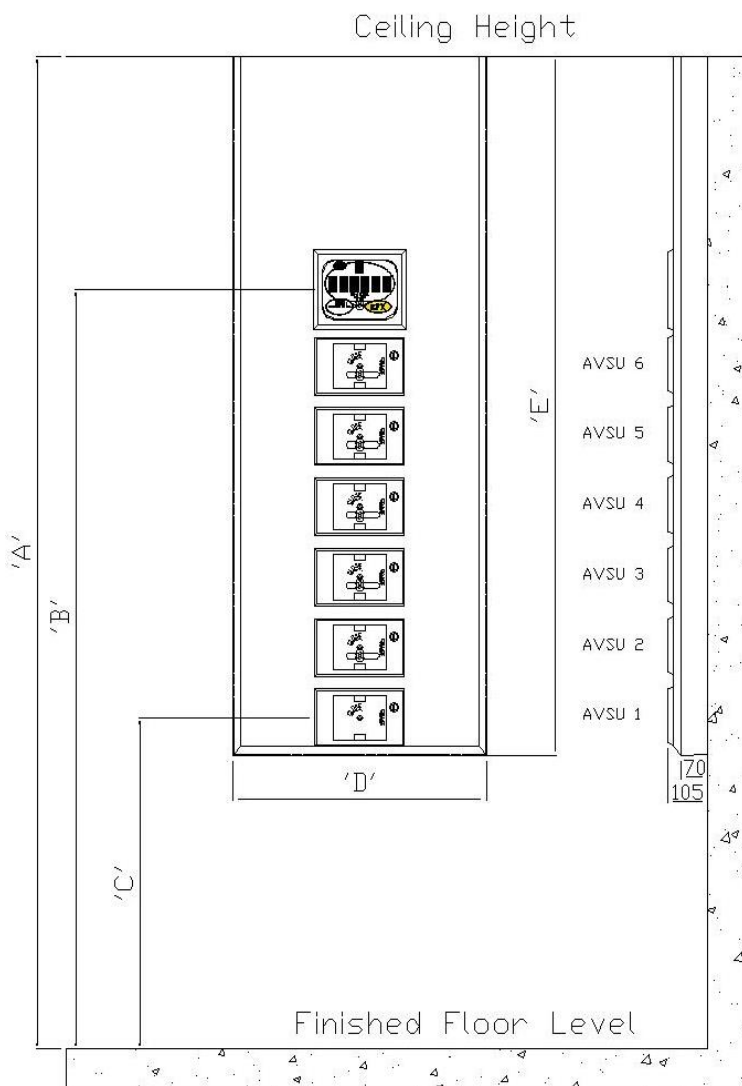

AVSU No.	Gas Type	Pipe Size
6		mm
5		mm
4		mm
3		mm
2		mm
1		mm
Notes:		
Alarm Manufacturer		
Model		
Logo Type		
'A' Dimension		
'B' Dimension		
'C' Dimension		
'D' Dimension		
'E' Dimension		
Signed By Precision UK		
Date		
Customer Signed		
Date		

Please return completed and signed off to enable production to begin, any delay may affect the agreed delivery date.